

UT305R Infrared Thermometer User Manual

Dear Users

Thank you for purchasing the new infrared thermometer. In order to use this product safely and correctly, please read this manual thoroughly, especially the *Precautions* part.

After reading this manual, it is recommended to keep the manual at an easily accessible place, preferably close to the device, for future reference.

Limited Warranty and Liability

Uni-Trend guarantees that the product is free from any defect in material and workmanship within one year from the purchase date. This warranty does not apply to damage caused by accident, negligence, misuse, modification, contamination or improper handling. The dealer shall not be entitled to give any other warranty on behalf of Uni-Trend. If you need warranty service within the warranty period, please contact your seller directly.

Uni-Trend will not be responsible for any special, indirect, incidental or subsequent damage or loss caused by using this device.

Introduction

The UT305R infrared thermometer (hereinafter referred to as the thermometer) can quickly and accurately determine the surface temperature by measuring the infrared energy radiated from the target surface. It is suitable for non-contact temperature measurement.

⚠️ Precautions

- To ensure proper use of the thermometer, please read this manual carefully before use.
- To ensure safety and accuracy of the thermometer, it should only be repaired by a qualified professional using original replacement parts.
- If the battery symbol on the LCD flashes, please replace the battery immediately to prevent inaccurate measurement.
- Inspect the case before using the thermometer. Do not use the thermometer if it appears damaged. Look for cracks or missing plastic.
- Avoid keeping the thermometer near high temperature environments for long periods.
- To ensure measurement accuracy, please use the thermometer in the operating environment [15°C~30°C, <85% RH (non-condensing)].
- Please use the thermometer indoors.
- The ambient temperature of the measured object must be stable, and it should not be measured in places with large airflow such as fans and air outlets.
- When changing to a new environment, please leave the thermometer for 30 minutes before use.
- When the measured object comes from a place with a large temperature difference from the measurement environment, keep it in the measurement environment for 10 to 30 minutes before measuring.
- Do not use the thermometer in places with strong sunlight or electromagnetic interference.
- After measuring extremely high or low temperature objects, please leave the thermometer for 10 minutes before next use.
- It is recommended to measure three times at a time, whichever is the most displayed set of data.
- Make the sensor window directly face the measured object during measurement, otherwise it will cause the measured temperature to be different from the actual temperature.
- Not for medical use

Specifications


Model	UT305R
Measuring range	32°C~42.9°C (89.6°F~109.2°F)
LCD size	30mm*30mm
LCD display	TN LCD
Accuracy	±0.3°C (±0.6°F)
Optimal measuring distance	5cm~10cm
Repeatability	0.3°C (0.6°F)
Response time	≤250ms (95% of reading)
Spectral response	8μm~14μm
Auto power off	15s
Low battery indication	√
High temperature LED alarm	>37.2°C: orange light alarm (≤37.2°C: green light)
High temperature audible alarm	>37.2°C: audible alarm
Data hold	√
Unit conversion (°C/°F)	√
Operating environment	15°C~30°C (59°F~86°F), <85% RH
Transportation/Storage environment	-20°C~60°C (-4°F~140°F), <85% RH
Battery type	9V battery (6F22)
Battery life	Continuous temperature measurement: ≥9 hours for the alkaline battery; ≥4 hours for the carbon battery
Accessories	Battery, user manual

Product Features

- Bright, easy-to-read, and high-contrast display
- With two-color (orange and green) LED and buzzer alarm functions
- With tripod mounting hole (¼ inch)

External Structure

1	Infrared sensor window
2	Trigger
3	Battery cover
4	Tripod mounting hole
5	LCD display
6	Buttons

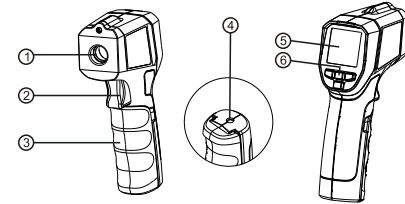

LCD Description

	Buzzer indicator	
HI OK LO	Temperature measurement alarm indicator	
	Low battery indicator	
SCAN	Temperature measurement indicator	
HOLD	Temperature hold indicator	
°C °F	Temperature unit indicator	
8888	Display of the measured temperature	

Operating Instructions

Power On

In the off state, short press the trigger to turn on the thermometer.

Power Off

In the HOLD mode, if there is no operation for 15s, the thermometer will automatically power off.

Manual Measurement

1. Pull and hold the trigger after aiming at the measured object. The SCAN icon will be flashing indicating that the target temperature is being measured. The measurement result will be updated on the LCD.
2. Release the trigger, the SCAN icon disappears, and the HOLD icon appears, indicating that the measurement has been stopped and the last measured value is held.
3. When the measured temperature exceeds 37.2°C, the HI icon is displayed and the orange light gives an alarm.

Temperature Unit Setting

In the HOLD interface, short press the SET button to enter the temperature unit setting interface, and switch between °C and °F by pressing the ▼ button or ▲ button.

Audible Alarm Setting

In the HOLD interface, short press the SET button twice to enter the audible alarm setting interface, and turn on/off the audible alarm by pressing the ▼ button or ▲ button.

Maintenance

General Maintenance

⚠️ As the thermometer is reusable apparatus, please pay attention to cleaning and maintenance before use. If it is not in use for a long time, please keep its lens clean and dust free.


1. Clean the case: Wipe dirt with a clean soft cloth or cotton swab dipped in medical alcohol or water.
2. Clean the lens: Use clean compressed air to blow off loose particles. Carefully wipe the surface with a cotton swab dipped in medical alcohol or water.

Battery Replacement

⚠️ If the thermometer is not in use for a long time, please remove the battery to prevent battery leakage. Dispose of used batteries properly in accordance with local regulations.

To replace the battery:

1. Open the battery cover.
2. Replace with a 9V battery (6F22), noting the polarity.
3. Close the battery cover.



Troubleshooting

Symptom	Cause	Action
HI appears	Measured value is greater than the maximum range	Stop measuring
LO appears	Measured value is less than the minimum range	Stop measuring
Err appears at booting	Exceeding the minimum or maximum operating temperature	Place the thermometer in a 0°C~50°C (32°F~122°F) environment for 30 minutes
Battery symbol flashes	Low battery	Replace the battery

UNI-T®


UNI-TREND TECHNOLOGY (CHINA) CO., LTD.

No. 6, Gong Ye Bei 1st Road,
Songsan Lake National High-Tech Industrial
Development Zone, Dongguan City,
Guangdong Province, China

Made in China



说明书菲林做货要求:

序号	项目	内容	
1	尺寸	尺寸: 285*210mm	折后: 105*71.25mm
2	材质	60g书纸	
3	颜色	单色印刷	
4	外观要求	完整清晰、版面整洁, 无斑墨、残损、毛边、刀线错位等缺陷。	
5	装订方式	无	
6	表面处理	无	
7	其它	无	
版本		0	
修改页码			
DWH 设计	宣浩	MODEL 机型:	Ut305R
CHK 审核		Part NO. 新: 110401109190X 物料编号: 旧:	
APPRO. 批准		 优利德科技(中国)有限公司 UNI-TREND TECHNOLOGY (CHINA) LIMITED	